


VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

OCT 28 2009

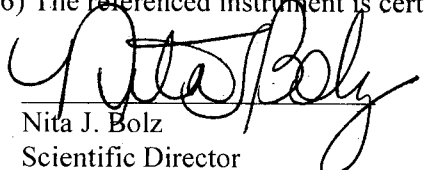
Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130179
Name		John T. Ostoj	ID# 4823 Date 10/24/09
A	Agency	AST	Phone #
Instrument Location		Soldotna	
Alco S/N		X124630	Target Value .079 High Pressure 900
B	Alco Test Value Average	.077	.077
		1 st Alco	2 nd Alco
Signature			
(OVER)			

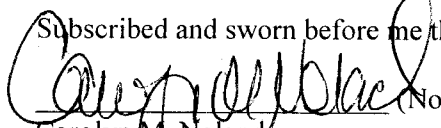
BMB
11/14/09

(Do Not write in the area below)

- I, Nita J. Bolz, after being first duly sworn, depose and state as follows:
- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
 - (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
 - (3) I am the Scientific Director of the State Breath Alcohol Program.
 - (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
 - (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
 - (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 3rd day of Dec, 2009.


Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

130179

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

Breath Test Record

Serial Number 130179 Model DataMaster
Location SLD0 AST/Soldotna

Subject Information

Last Name Voc O.L. # VOC
First Name Test

Operator Information

Operator Name Ostoja/John/T Case VOC
Operator # 4823 Department SLD0

Test Results

Alco Target .079 Alco Serial X124630
Nominal 0.078 Barometer 29.62 Test Type V
Dry Gas 1 0.077 Time: 19:58:20 Test Date 10/24/2009
Subject Alcohol 0.000 Time: 19:59:36 Test Time 19:56:35
Dry Gas 2 0.077 Time: 20:00:46 Report Y

DIAGNOSTIC CHECK

Diagnostic Test Record

Serial Number 130179 Model DataMaster
Location SLD0 AST/Soldotna

Diagnostic Test Results

Test Date 10/24/2009 Computer Okay
Test Time 19:53:20 Program Okay
Software Date 02/20/2001
Sample Chamber (C) 49
Breath Tube (C) 41
Barometer (in) 29.62
Flow Detector Okay
High Speed Pump Okay
Detector Okay
Filter Okay
Quartz Okay
Calibration Okay